


Sample Name: 113671

=====

Acq. Operator : Z	Seq. Line : 2
Acq. Instrument : instr1	Location : Vial 12
	Inj Volume : 15.000 µl
Different Inj Volume from Sequence !	Actual Inj Volume : 5.000 µl

Additional Info : Peak(s) manually integrated

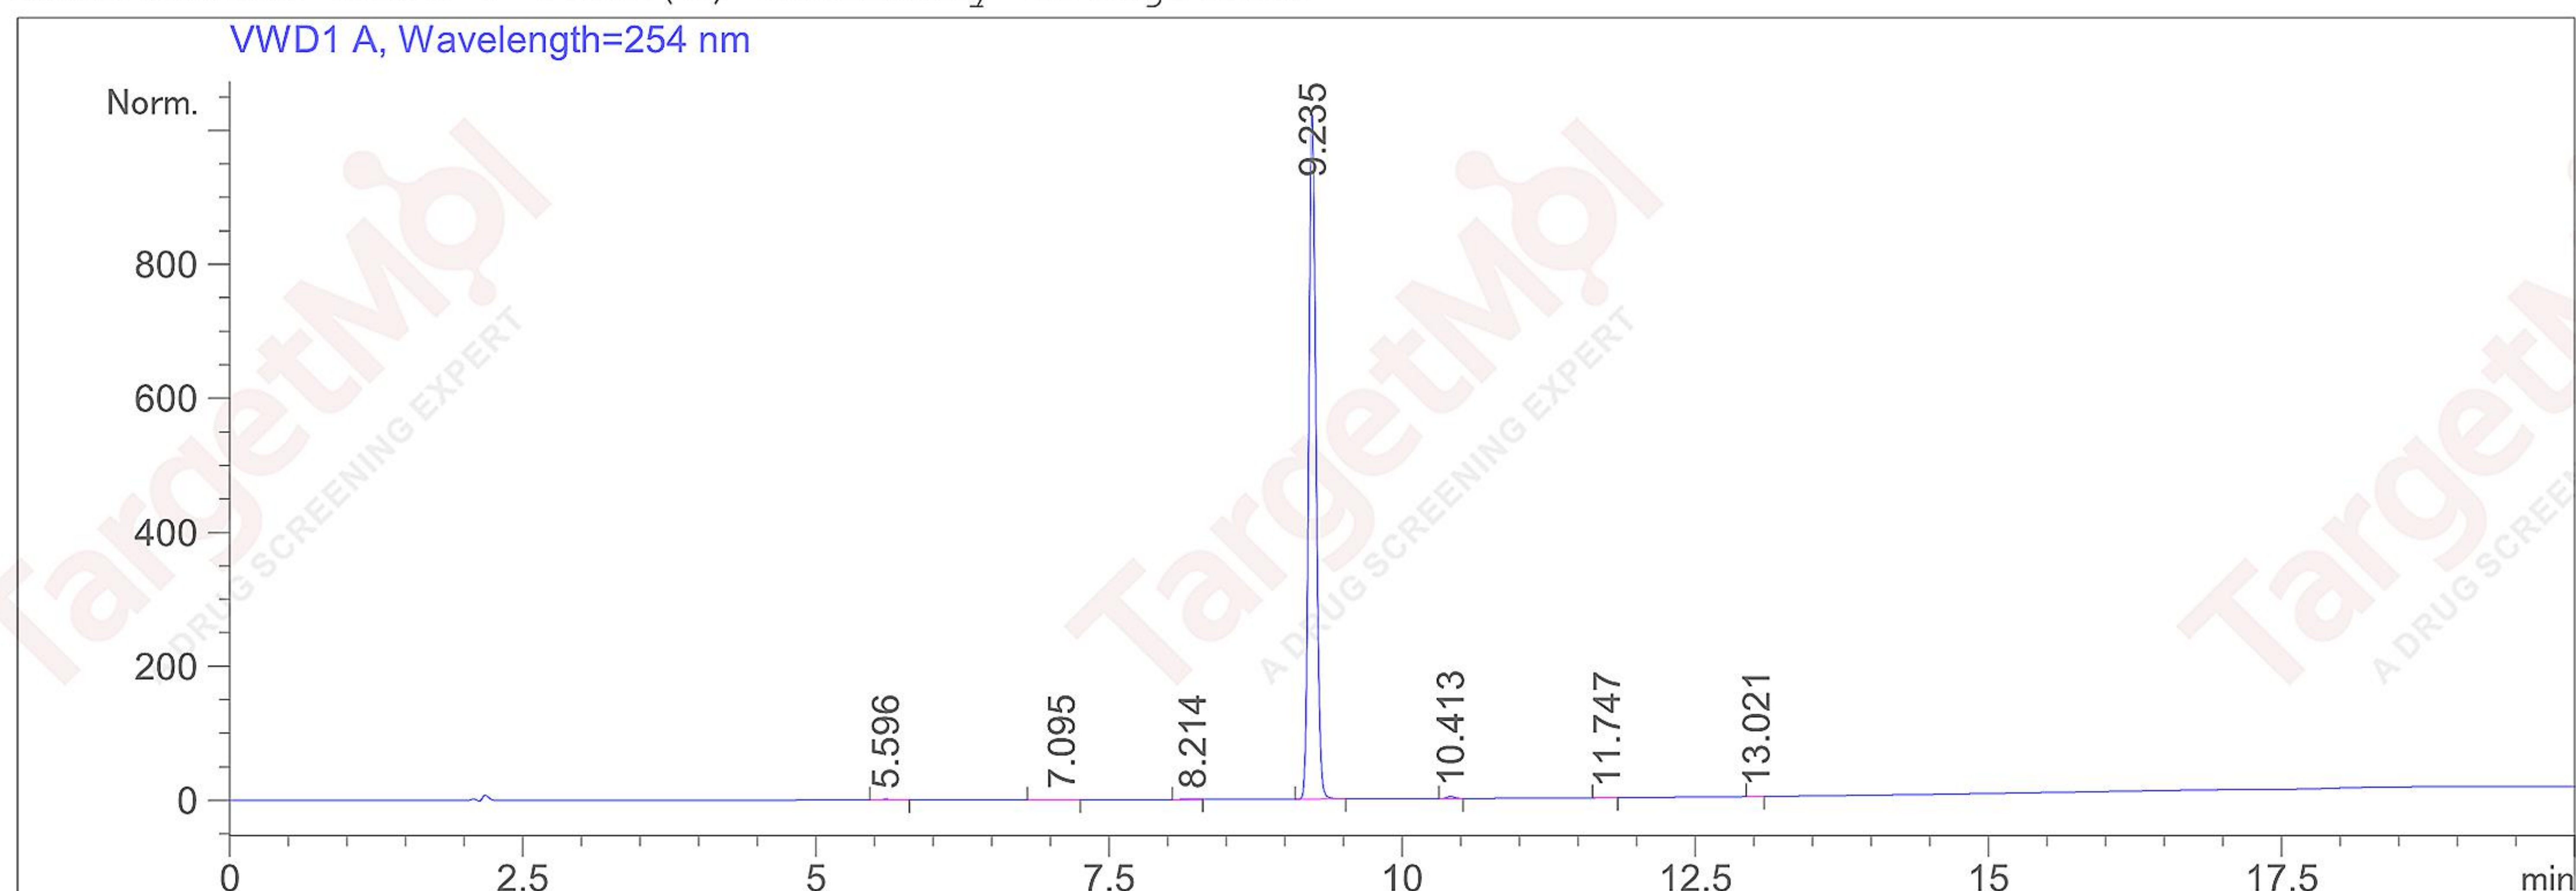

=====  
Area Percent Report  
=====

Sorted By : Signal  
Multiplier: : 1.0000  
Dilution: : 1.0000  
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=254 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	5.596	BB	0.0784	4.77766	9.53709e-1	0.1085
2	7.095	BB	0.0784	2.13225	4.11869e-1	0.0484
3	8.214	BB	0.0987	1.19951	1.71354e-1	0.0272
4	9.235	BB	0.0671	4377.64648	1019.83929	99.4055
5	10.413	BB	0.0648	14.06147	3.36191	0.3193
6	11.747	BB	0.0731	2.70616	5.83314e-1	0.0615
7	13.021	BB	0.0677	1.30579	3.00198e-1	0.0297

Totals : 4403.82933 1025.62165

=====  
\*\*\* End of Report \*\*\*  
=====